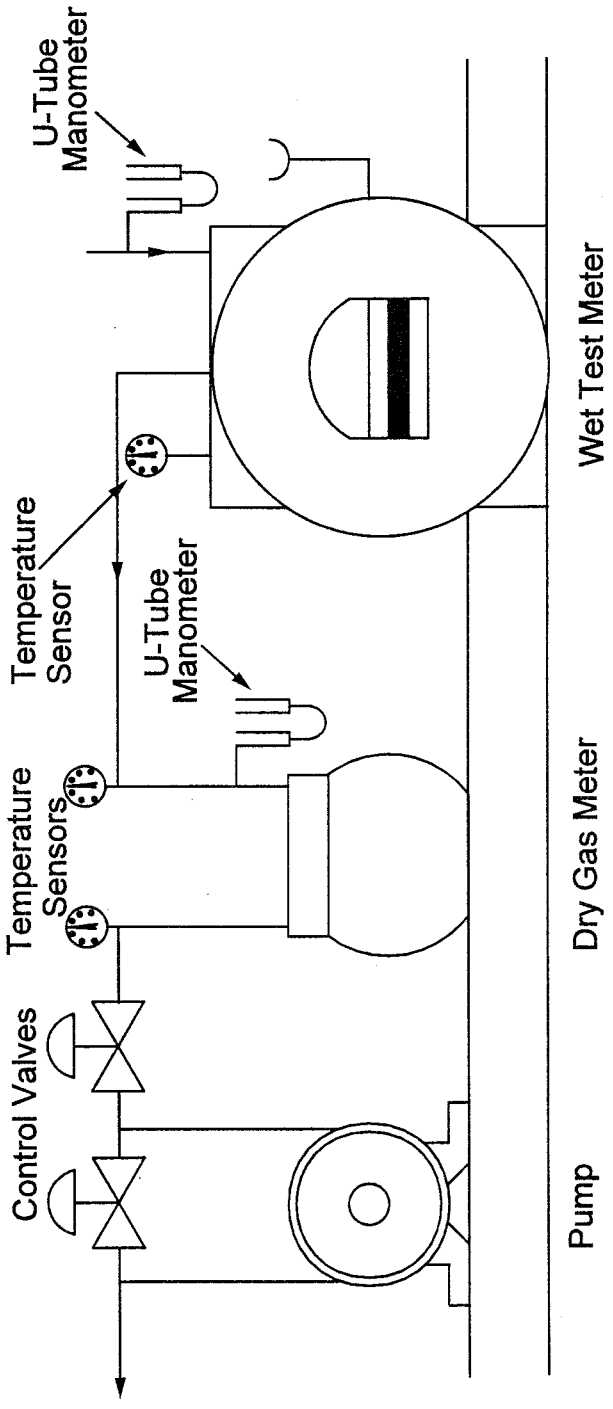

Figure 5-7. Equipment Arrangement for Dry Gas Meter Calibration.