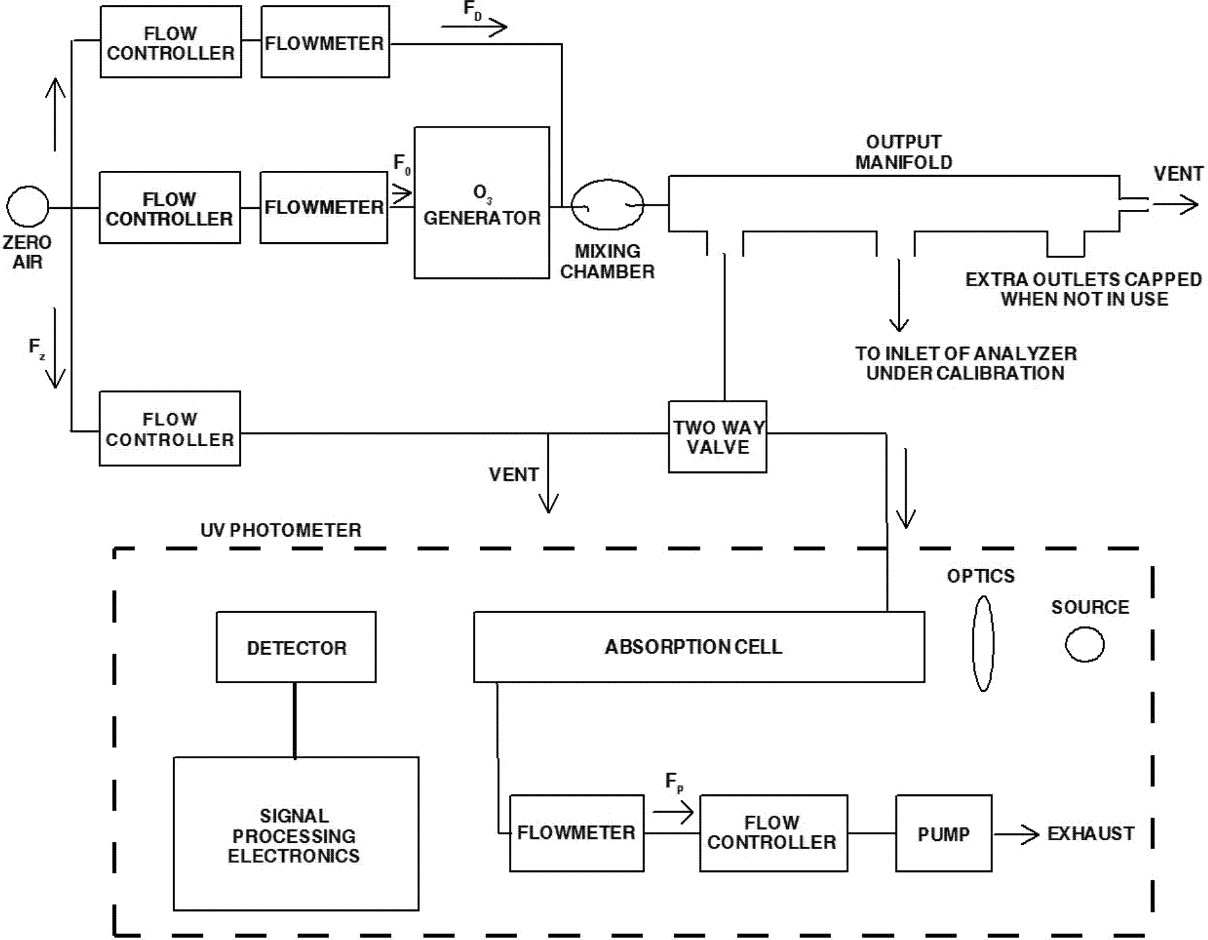

Figure 3. Schematic diagram of a typical UV photometric calibration system (Option 1).