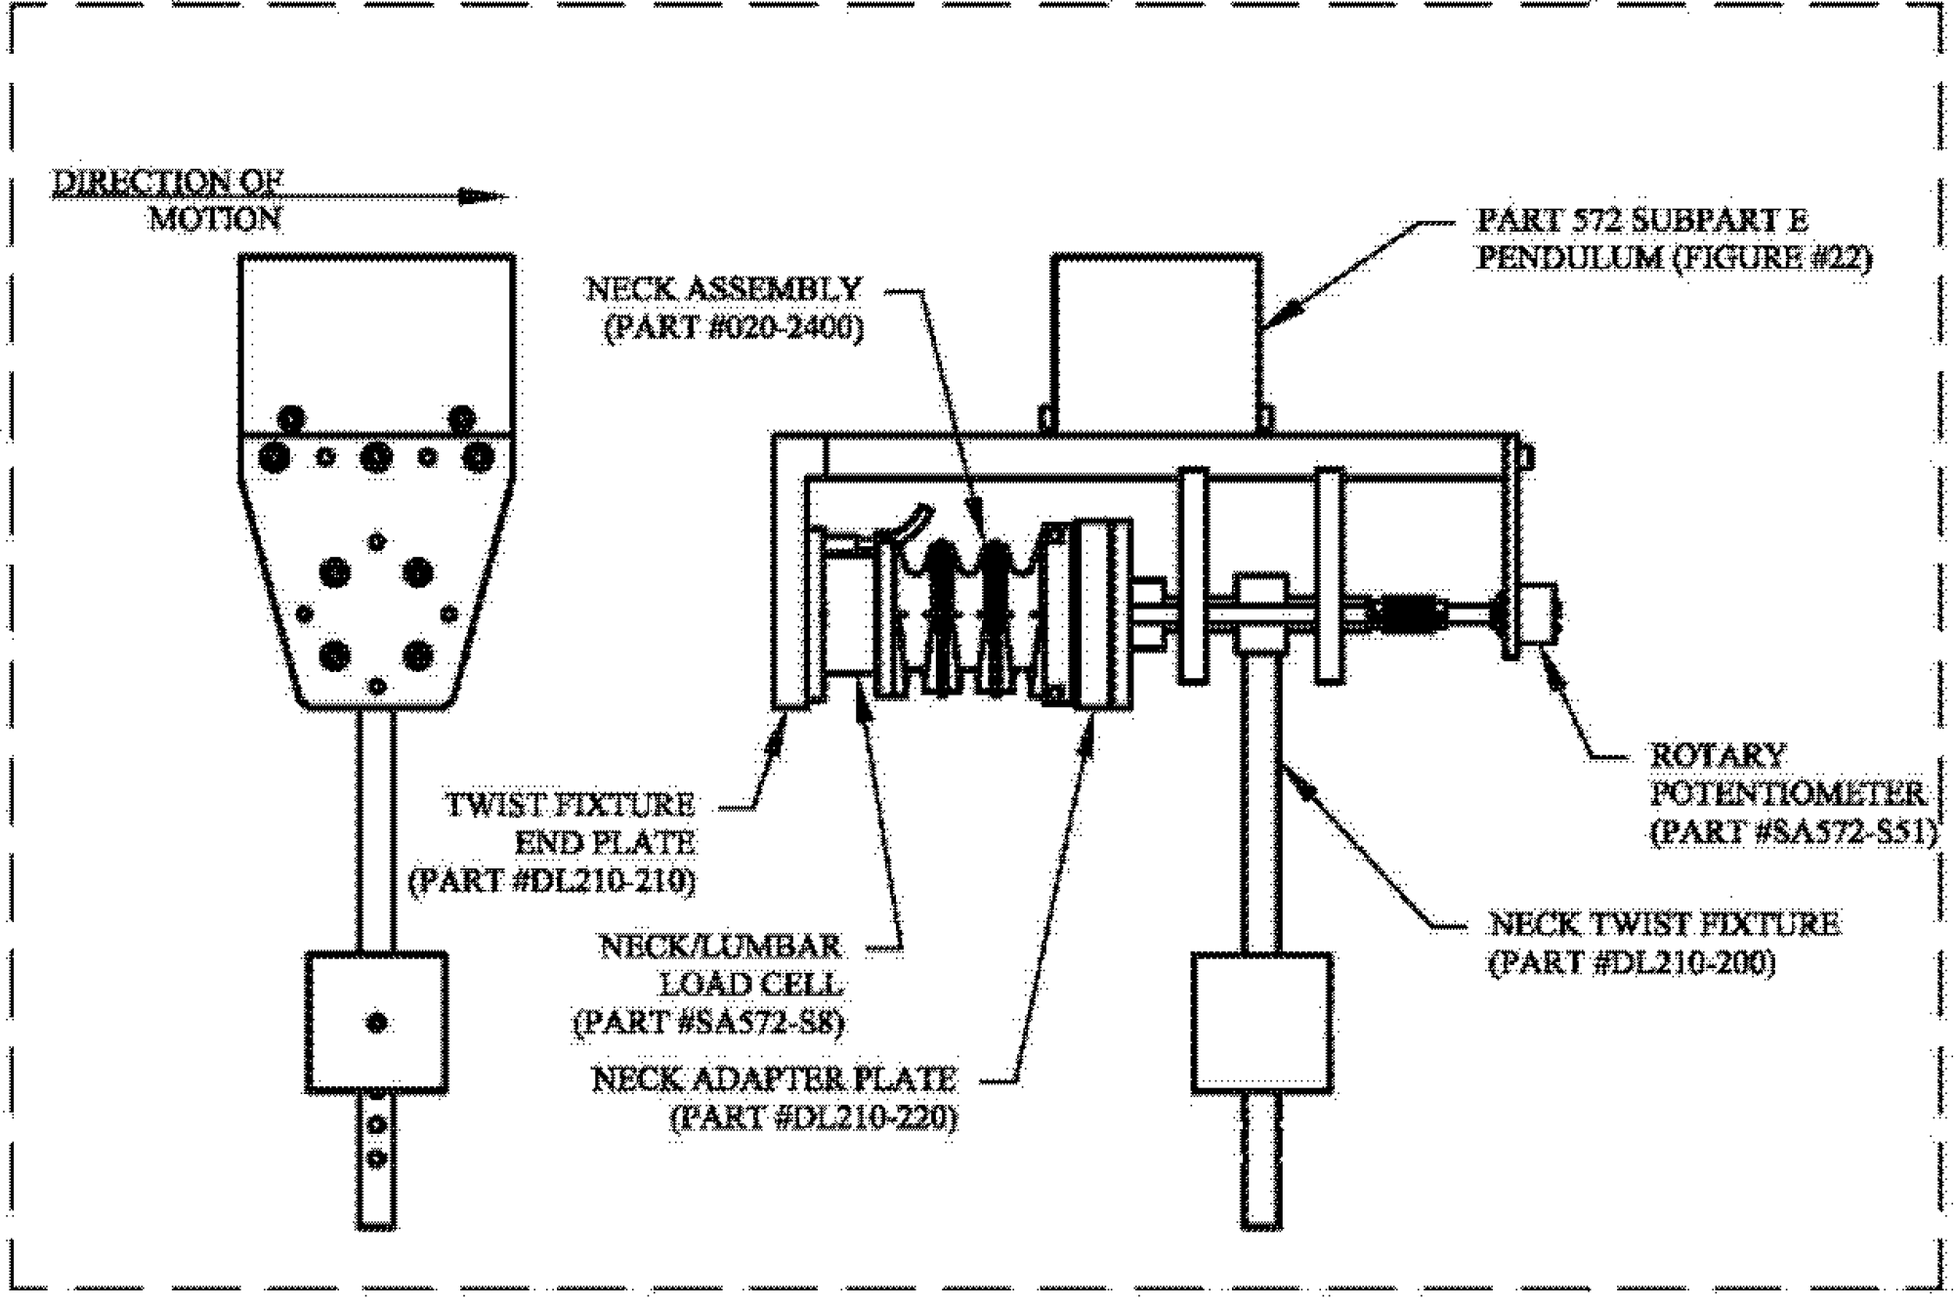

Figure W5. Neck torsion test set-up specifications.