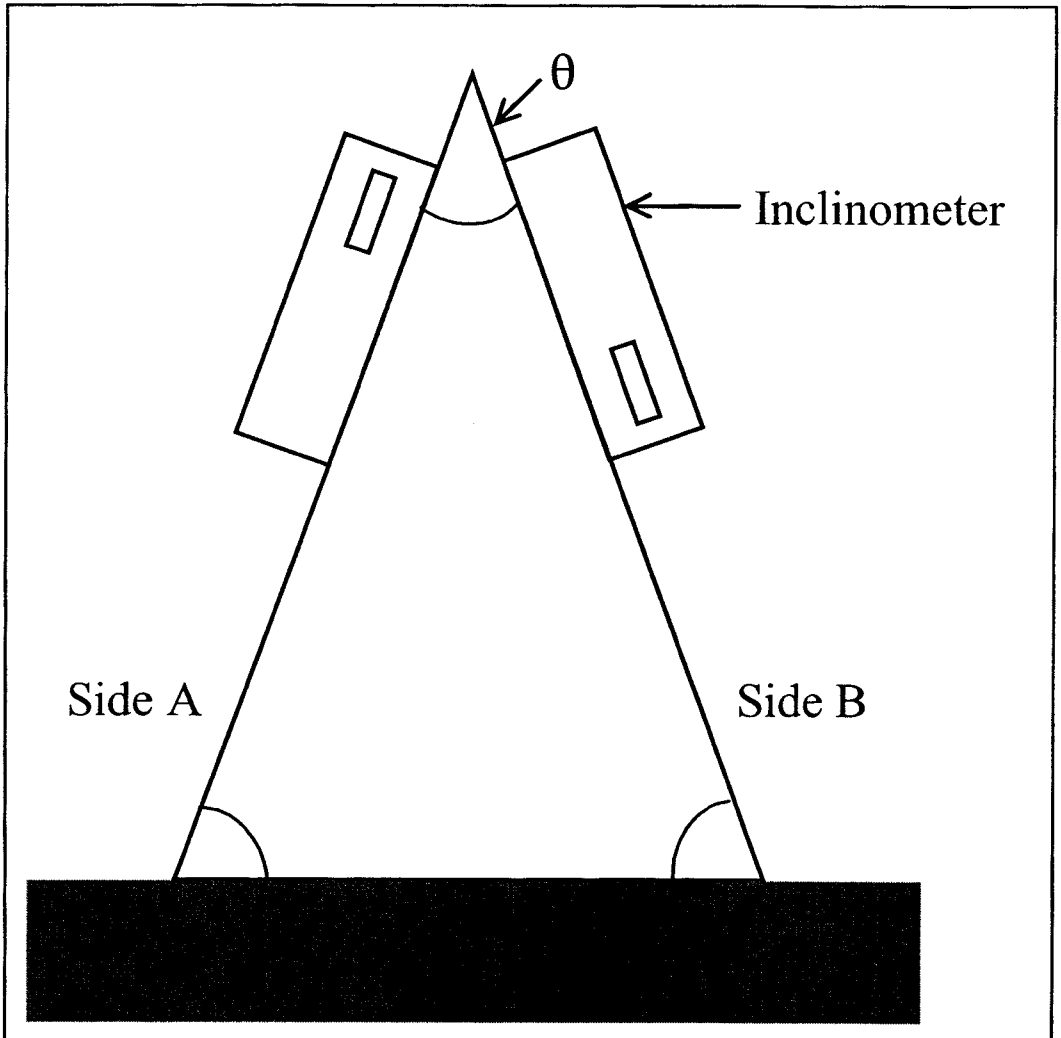

Figure 2G-9. Triangular block used for digital inclinometer calibration.